


## ENDOSCOPIC ULTRASOUND NEEDLE (EUS)

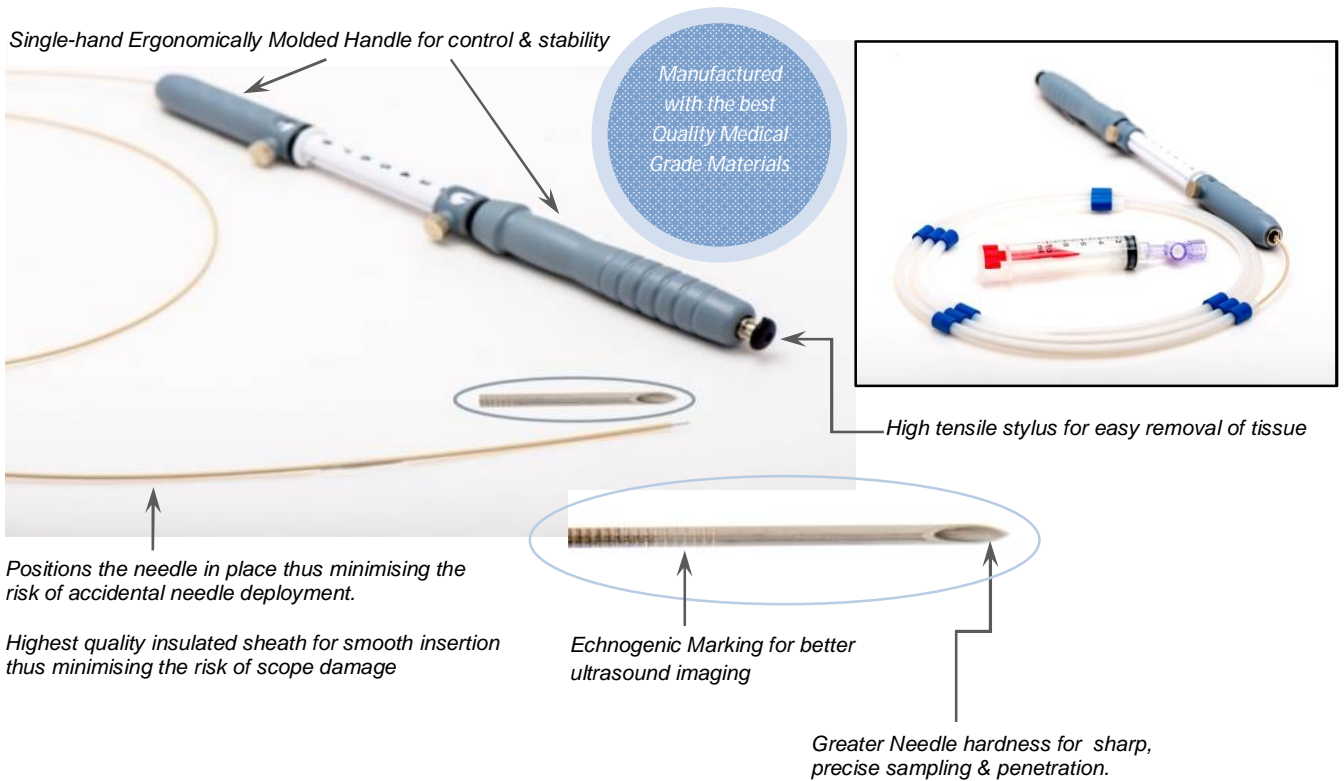

### VARIANTS :

CODE NO	DIAMETER	WORKING LENGTH	EXPOSED TIP LENGTH	OUTER SHEATH OD
GEUS22-01	22 Fr	1400 mm	80 mm	1.77
GEUS22-02	22 Fr	700 mm	80 mm	1.77
GEUS19-01	19 Fr	1400 mm	80 mm	1.77
GEUS19-02	19 Fr	700 mm	80 mm	1.77

### DEVICE DESCRIPTION :

Glowtronics Endoscopic Ultrasound Needle is a sterile single use device. It is an endoscopic needle that can be coupled to the biopsy channel of a Echoendoscope and it is used to collect samples from lesions within and adjacent to the digestive system's major lumen that can be targeted through echoendoscope.

### INTENDED USE :

This device is used to sample targeted submucosal gastrointestinal lesions through the accessory channel of an ultrasound endoscope (Echoendoscope).

### WARNING :

This device should only be used by or under supervision of qualified endoscopists thoroughly trained in Endoscopic procedures. A complete understanding of the technical principles, clinical applications and risks associated in endoscopic procedures is necessary before using this device. Ensure sterilization of the device before use.

### CAUTION :

These devices are for Single - use ONLY.  
 Check expiry date prior to use. Do not use after expiry date.  
 Do not Reuse, Re - process or Re-sterilize.  
 Do not use if package is opened or damaged when received.  
 This device must be stored in dry & cool condition, away from extreme temperature.  
 Use of this device for any other purpose other than the stated intended use is neither advised nor recommended.



Glowtronics Pvt Ltd

1D, Hootagalli Industrial Area,

Mysore – 570 018, India Tel: +91-821-240-2461/2462

Email: [marketing@glowtronics.com](mailto:marketing@glowtronics.com) Website: [www.glowtronics.com](http://www.glowtronics.com)



intertek



intertek

